

Para 12[®] Plus Retics

Instrument/Serial Number - Abbott CELL-DYN[®] 3200

Lab Acct Number: 00100
 SAMPLE LAB REPORT
 1234 MAIN STREET
 ANYTOWN, NE USA 68130

Lot Number 9075
 Instrument Number 339
 Shift 1

Report Date 06/15/2009
 Date Received 06/03/2009
 Date From 04/01/2009
 Date To 05/29/2009

Interpretive Comments

THIS PAGE CONTAINS GENERAL AND SPECIFIC NOTES RELATIVE TO THE DATA SUBMITTED BY YOUR LAB

REVIEWED BY: _____ DATE: _____

DUE DATE FOR NEXT DATA SUBMISSION: 08/10/2009

GENERAL REPORT:

This report separates data in the left and right columns to provide calculations for the current cycle submission, and cumulative calculations over the dating of the lot. On the first submission for each lot, the Current and Cumulative data will be the same. The CV may be large on some parameters due to the small numeric value, and/or the small number of significant digits reported. Any data that falls outside of your lab's 3 SD or is significantly different from the assay mean will be excluded from peer group calculations. Excluded values are listed on the following page and are highlighted with an asterisk (*) in the Customer Data section. Levey-Jennings graphs are also provided for selected parameters.

S.D.I. REPORT:

This report is a graphical presentation of your laboratory's data on the current lot. The S.D.I. allows you to inspect results from many different tests at the same time, without having to consider different units and the actual magnitude of the change in the units of the test. In general, any S.D.I. of 2.0 or greater deserves some attention because your method shows a systematic difference from the group. The S.D.I. report is provided for selected parameters.

HISTORICAL DATA COMPARISON REPORT:

This report is a chronological presentation of your laboratory's data over the last six submissions. These calculations assist you in complying with CLIA regulations for establishing your laboratory's means and ranges on controls. The 2 SD is provided for all levels and parameters reported over the last six submissions. The historical CV is provided to monitor your method and instrument's performance over multiple lots. The historical SD and CV are comprised of all data points submitted, including values outside of the group 3 SD. These values may differ slightly from your monthly reports.

STANDARD CALCULATIONS PROVIDED:

Mean	SD	CV = (SD ÷ Mean) x 100	S.D.I. = $\frac{\text{Your Mean} - \text{Peer Group Mean}}{\text{Peer Group SD}}$
------	----	------------------------	---

For a detailed explanation of the STATS[®] report format or more information regarding QC concepts, please visit Streck online at: <http://www.streck.com/services/stats.asp>

Para 12[®] Plus Retics

Instrument/Serial Number - Abbott CELL-DYN[®] 3200

Lab Acct Number: 00100
SAMPLE LAB REPORT
1234 MAIN STREET
ANYTOWN, NE USA 68130

Lot Number 9075
Instrument Number 339
Shift 1

Report Date 06/15/2009
Date Received 06/03/2009
Date From 04/01/2009
Date To 05/29/2009

DATA EXCLUDED FROM PEER GROUP MEAN:

No data excluded from calculations.

Para 12[®] Plus Retics

Instrument/Serial Number - Abbott CELL-DYN[®] 3200

Lab Acct Number: 00100
 SAMPLE LAB REPORT
 1234 MAIN STREET
 ANYTOWN, NE USA 68130

Lot Number 9075
 Instrument Number 339
 Shift 1

Report Date 06/15/2009
 Date Received 06/03/2009
 Date From 04/01/2009
 Date To 05/29/2009

General Report

Current Submission
 Number of Labs: 10

Low 90750260

Cumulative Submissions
 Total Number Of Labs: 22

Para-Meter	Assay Mean	Your Mean	Your SD	Your CV	Group Mean	Group N	Group SD	Group CV	S.D.I.	Your Mean	Your SD	Your CV	Group Mean	Group N	Group SD	Group CV	S.D.I.
WOC	3.1	3.1	0.06	1.97	3.1	581	0.08	2.67	-0.03	3.1	0.06	1.97	3.0	1183	0.09	3.00	0.04
NEUT#	1.5	1.6	0.05	2.79	1.6	576	0.07	4.12	0.16	1.6	0.05	2.79	1.6	999	0.07	4.42	0.17
NEUT%	49.3	53.0	1.04	1.96	52.6	552	1.61	3.07	0.26	53.0	1.04	1.96	52.4	1129	1.73	3.31	0.35
LYM#	1.1	1.0	0.05	4.95	1.0	569	0.06	5.64	-0.01	1.0	0.05	4.95	1.0	987	0.05	5.07	-0.03
LYM%	34.0	33.1	1.15	3.47	33.0	543	1.39	4.20	0.06	33.1	1.15	3.47	33.1	1112	1.39	4.19	0.02
MONO#	0.3	0.2	0.02	8.44	0.2	564	0.03	10.77	-0.20	0.2	0.02	8.44	0.2	982	0.03	11.48	-0.13
MONO%	8.8	7.8	0.59	7.55	7.9	545	0.83	10.40	-0.16	7.8	0.59	7.55	7.9	1129	1.12	14.30	-0.04
EOS#	0.1	0.1	0.01	12.50	0.1	575	0.01	13.33	-0.11	0.1	0.01	12.50	0.1	997	0.01	13.39	-0.13
EOS%	3.0	2.1	0.24	11.43	2.1	553	0.28	13.03	-0.10	2.1	0.24	11.43	2.1	1141	0.28	13.28	-0.14
BASO#	0.2	0.1	0.03	21.55	0.1	572	0.03	20.53	-0.51	0.1	0.03	21.55	0.1	988	0.03	20.92	-0.64
BASO%	5.0	3.8	0.77	20.05	4.3	550	0.82	19.36	-0.51	3.8	0.77	20.05	4.4	1135	1.02	23.36	-0.51
RBC	2.92	2.92	0.03	1.03	2.92	582	0.05	1.81	0.05	2.92	0.03	1.03	2.92	1195	0.06	2.00	0.02
HGB	7.5	7.0	0.19	2.73	7.3	581	0.28	3.77	-1.34	7.0	0.19	2.73	7.3	1194	0.25	3.43	-1.50
HCT	21.8	21.7	0.23	1.04	21.5	573	0.45	2.10	0.52	21.7	0.23	1.04	21.3	1184	0.50	2.36	0.85
MCV	74.5	74.5	0.59	0.79	73.6	582	1.02	1.38	0.83	74.5	0.59	0.79	72.9	1197	1.29	1.77	1.21
MCH	25.7	23.8	0.72	3.02	25.1	581	1.01	4.01	-1.26	23.8	0.72	3.02	25.1	1192	1.01	4.00	-1.27
MCHC	34.4	32.1	0.98	3.06	34.1	578	1.58	4.62	-1.31	32.1	0.98	3.06	34.5	1189	1.47	4.26	-1.64
RDW%	12.6	13.2	0.20	1.51	13.1	583	0.50	3.84	0.12	13.2	0.20	1.51	12.9	1197	0.67	5.16	0.44
PLT	79	83	5.20	6.24	84	581	5.12	6.08	-0.17	83	5.20	6.24	84	1196	5.90	7.06	-0.03

Para 12[®] Plus Retics

Instrument/Serial Number - Abbott CELL-DYN[®] 3200

Lab Acct Number: 00100
 SAMPLE LAB REPORT
 1234 MAIN STREET
 ANYTOWN, NE USA 68130

Lot Number 9075
 Instrument Number 339
 Shift 1

Report Date 06/15/2009
 Date Received 06/03/2009
 Date From 04/01/2009
 Date To 05/29/2009

Current Submission
 Number of Labs: 13

Normal 90750261

Cumulative Submissions
 Total Number Of Labs: 28

Para-Meter	Assay Mean	Your Mean	Your SD	Your CV	Group Mean	Group N	Group SD	Group CV	S.D.I.	Your Mean	Your SD	Your CV	Group Mean	Group N	Group SD	Group CV	S.D.I.
WOC	7.1	7.1	0.10	1.42	7.1	715	0.14	2.01	0.05	7.1	0.10	1.42	7.0	1520	0.17	2.38	0.20
NEUT#	3.9	4.2	0.08	1.80	4.1	707	0.13	3.24	0.39	4.2	0.08	1.80	4.1	1161	0.14	3.47	0.42
NEUT%	55.2	58.9	0.67	1.14	58.3	685	1.54	2.64	0.43	58.9	0.67	1.14	58.1	1462	1.61	2.78	0.50
LYM#	1.9	1.8	0.06	3.43	1.8	703	0.07	3.86	-0.04	1.8	0.06	3.43	1.8	1157	0.07	3.98	-0.02
LYM%	26.2	26.0	0.77	2.96	26.1	679	0.83	3.20	-0.11	26.0	0.77	2.96	26.2	1452	0.95	3.63	-0.17
MONO#	0.8	0.6	0.03	5.31	0.6	705	0.06	9.35	-0.11	0.6	0.03	5.31	0.6	1161	0.07	10.62	0.03
MONO%	10.7	9.1	0.47	5.19	9.2	681	0.85	9.26	-0.14	9.1	0.47	5.19	9.1	1461	0.93	10.11	-0.09
EOS#	0.2	0.2	0.01	7.41	0.2	710	0.02	7.98	0.01	0.2	0.01	7.41	0.2	1166	0.02	8.99	0.06
EOS%	2.6	2.7	0.20	7.46	2.7	685	0.20	7.65	0.01	2.7	0.20	7.46	2.7	1471	0.21	7.83	-0.01
BASO#	0.3	0.2	0.02	9.75	0.3	703	0.05	18.24	-0.63	0.2	0.02	9.75	0.3	1157	0.05	19.73	-0.64
BASO%	4.5	3.3	0.32	9.61	3.8	678	0.68	18.06	-0.63	3.3	0.32	9.61	3.8	1465	0.79	20.74	-0.62
RBC	4.24	4.27	0.04	0.94	4.27	717	0.06	1.39	-0.01	4.27	0.04	0.94	4.27	1529	0.06	1.51	0.05
HGB	12.0	12.2	0.23	1.88	12.1	713	0.21	1.77	0.75	12.2	0.23	1.88	12.0	1521	0.22	1.85	0.95
HCT	32.3	32.8	0.39	1.19	32.5	717	0.64	1.98	0.48	32.8	0.39	1.19	32.1	1526	0.79	2.46	0.81
MCV	76.1	76.7	0.63	0.82	76.0	712	1.08	1.42	0.63	76.7	0.63	0.82	75.3	1527	1.53	2.04	0.91
MCH	28.3	28.6	0.59	2.06	28.2	712	0.53	1.88	0.68	28.6	0.59	2.06	28.2	1521	0.58	2.06	0.77
MCHC	37.2	37.3	0.87	2.33	37.2	716	0.76	2.05	0.18	37.3	0.87	2.33	37.4	1527	0.86	2.31	-0.12
RDW%	10.6	11.4	0.20	1.75	11.3	716	0.38	3.35	0.35	11.4	0.20	1.75	11.1	1530	0.51	4.63	0.67
PLT	236	239	9.10	3.81	241	715	10.26	4.26	-0.23	239	9.10	3.81	240	1528	11.96	4.98	-0.11

Para 12[®] Plus Retics

Instrument/Serial Number - Abbott CELL-DYN[®] 3200

Lab Acct Number: 00100
 SAMPLE LAB REPORT
 1234 MAIN STREET
 ANYTOWN, NE USA 68130

Lot Number 9075
 Instrument Number 339
 Shift 1

Report Date 06/15/2009
 Date Received 06/03/2009
 Date From 04/01/2009
 Date To 05/29/2009

Current Submission
 Number of Labs: 12

High 90750262

Cumulative Submissions
 Total Number Of Labs: 26

Para-Meter	Assay Mean	Your Mean	Your SD	Your CV	Group Mean	Group N	Group SD	Group CV	S.D.I.	Your Mean	Your SD	Your CV	Group Mean	Group N	Group SD	Group CV	S.D.I.
WOC	15.7	15.6	0.25	1.60	15.7	688	0.36	2.29	-0.21	15.6	0.25	1.60	15.6	1483	0.43	2.78	-0.05
NEUT#	9.4	10.1	0.22	2.18	10.0	682	0.36	3.55	0.21	10.1	0.22	2.18	10.0	1124	0.39	3.92	0.20
NEUT%	59.8	64.6	0.74	1.14	63.8	656	1.72	2.70	0.47	64.6	0.74	1.14	63.7	1425	1.80	2.82	0.50
LYM#	3.0	3.0	0.10	3.36	3.0	681	0.14	4.75	-0.18	3.0	0.10	3.36	3.0	1127	0.17	5.70	-0.17
LYM%	19.1	19.1	0.60	3.14	19.2	657	0.86	4.49	-0.11	19.1	0.60	3.14	19.2	1425	0.92	4.78	-0.15
MONO#	1.8	1.5	0.10	6.54	1.6	682	0.15	9.85	-0.21	1.5	0.10	6.54	1.5	1123	0.17	10.81	-0.05
MONO%	11.3	9.8	0.66	6.71	10.0	657	1.00	10.02	-0.15	9.8	0.66	6.71	9.9	1422	1.02	10.33	-0.04
EOS#	0.5	0.5	0.03	6.38	0.5	684	0.03	6.67	-0.20	0.5	0.03	6.38	0.5	1127	0.03	6.83	-0.21
EOS%	3.0	3.0	0.17	5.61	3.0	659	0.18	6.04	-0.06	3.0	0.17	5.61	3.1	1428	0.19	6.10	-0.11
BASO#	0.8	0.5	0.04	7.55	0.6	681	0.12	19.93	-0.76	0.5	0.04	7.55	0.6	1126	0.14	22.06	-0.76
BASO%	5.4	3.4	0.29	8.55	4.0	656	0.78	19.62	-0.73	3.4	0.29	8.55	4.1	1427	0.86	21.10	-0.81
RBC	5.08	5.08	0.06	1.18	5.12	690	0.09	1.77	-0.42	5.08	0.06	1.18	5.11	1479	0.09	1.84	-0.31
HGB	16.0	16.5	0.28	1.70	16.2	690	0.34	2.09	1.05	16.5	0.28	1.70	16.0	1479	0.34	2.12	1.43
HCT	41.0	41.3	0.66	1.60	41.3	691	0.85	2.06	-0.06	41.3	0.66	1.60	40.9	1483	1.08	2.65	0.39
MCV	80.7	81.3	0.70	0.86	80.7	688	1.14	1.41	0.45	81.3	0.70	0.86	79.9	1486	1.70	2.12	0.78
MCH	31.5	32.5	0.50	1.54	31.6	688	0.75	2.39	1.23	32.5	0.50	1.54	31.4	1482	0.76	2.42	1.48
MCHC	39.0	40.0	0.72	1.80	39.1	689	0.92	2.35	0.98	40.0	0.72	1.80	39.2	1484	0.91	2.32	0.82
RDW%	9.9	10.8	0.19	1.75	10.7	689	0.37	3.41	0.34	10.8	0.19	1.75	10.5	1486	0.46	4.33	0.71
PLT	585	575	19.50	3.39	585	690	22.16	3.79	-0.45	575	19.50	3.39	583	1485	26.77	4.59	-0.30

++CV's greater than 100 may be due to the small numeric value and the inability of the analyzer to report out results to more significant digits.

Para 12[®] Plus Retics


Instrument/Serial Number - Abbott CELL-DYN[®] 3200

Lab Acct Number: 00100
 SAMPLE LAB REPORT
 1234 MAIN STREET
 ANYTOWN, NE USA 68130

Lot Number 9075
 Instrument Number 339
 Shift 1

Report Date 06/15/2009
 Date Received 06/03/2009
 Date From 04/01/2009
 Date To 05/29/2009

S.D.I. Reports

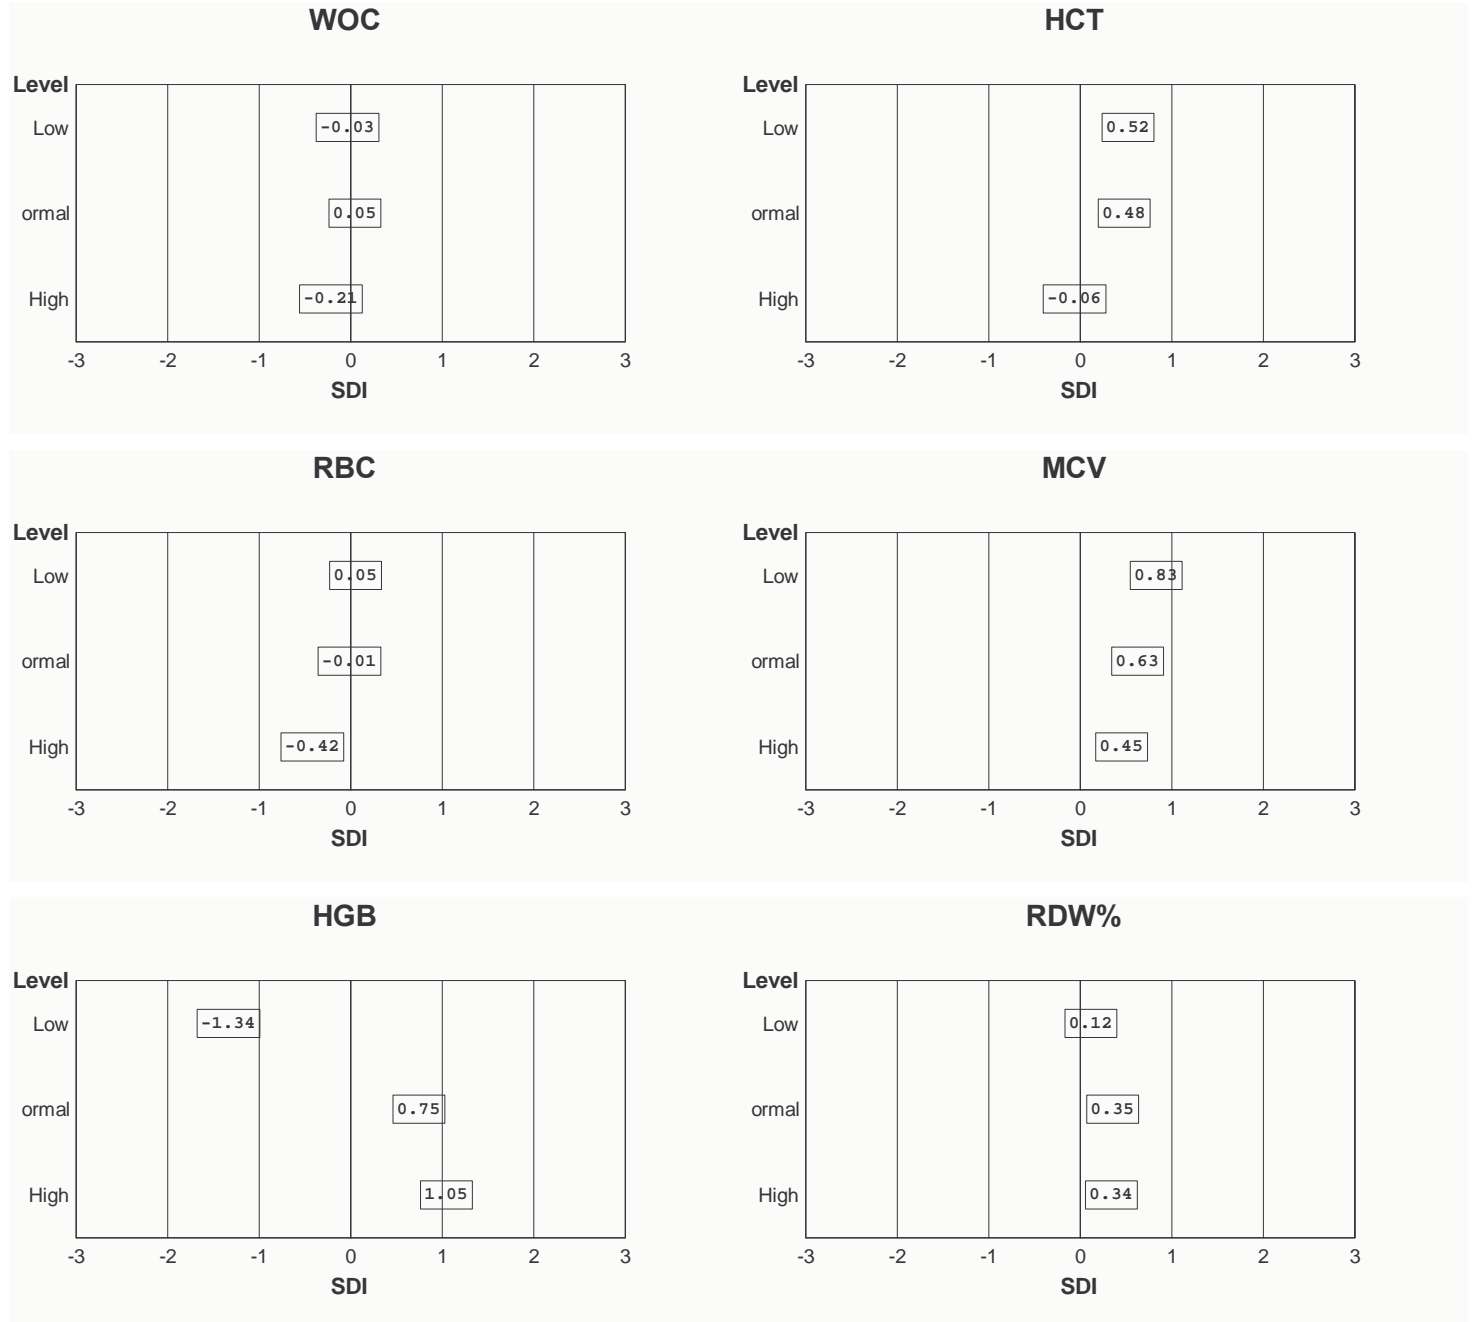


Para 12[®] Plus Retics

Instrument/Serial Number - Abbott CELL-DYN[®] 3200

Lab Acct Number: 00100
SAMPLE LAB REPORT
1234 MAIN STREET
ANYTOWN, NE USA 68130

Lot Number 9075
Instrument Number 339
Shift 1

Report Date 06/15/2009
Date Received 06/03/2009
Date From 04/01/2009
Date To 05/29/2009

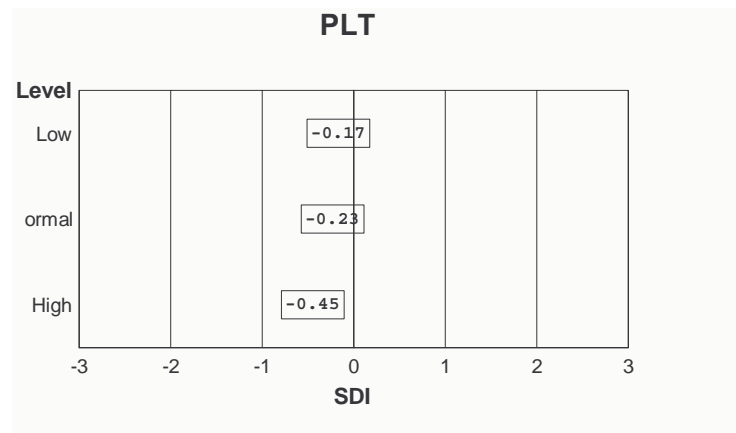

Para 12[®] Plus Retics

Instrument/Serial Number - Abbott CELL-DYN[®] 3200

Lab Acct Number: 00100
 SAMPLE LAB REPORT
 1234 MAIN STREET
 ANYTOWN, NE USA 68130

Lot Number 9075
 Instrument Number 339
 Shift 1

Report Date 06/15/2009
 Date Received 06/03/2009
 Date From 04/01/2009
 Date To 05/29/2009

Historical Data Comparison Report - Last 6 Submissions

Low

Lot #s	SD						Historical		CV					
	8273	8273	8329	9019	9019	9075	SD	2 SD	8273	8273	8329	9019	9019	9075
WOC	0.07	0.07	0.07	0.07	0.06	0.06	0.07	0.1	2.23	2.23	2.23	2.35	2.03	1.97
NEUT#	0.05	0.04	0.04	0.05	0.05	0.05	0.05	0.1	3.16	2.71	2.50	3.16	3.18	2.79
NEUT%	1.11	0.94	1.13	1.19	1.01	1.04	1.07	2.1	2.16	1.82	2.21	2.24	1.89	1.96
LYM#	0.06	0.05	0.05	0.09	0.05	0.05	0.06	0.1	5.77	4.49	4.76	9.09	5.26	4.95
LYM%	1.25	1.08	0.88	1.12	1.02	1.15	1.08	2.2	3.80	3.32	2.64	3.45	3.17	3.47
MONO#	0.03	0.02	0.05	0.05	0.04	0.02	0.03	0.1	8.67	7.28	18.52	21.74	16.67	8.44
MONO%	0.84	0.70	0.67	0.63	0.76	0.59	0.70	1.4	8.80	7.28	7.44	7.62	9.18	7.55
EOS#	0.01	0.01	0.01	0.01	0.01	0.01	0.01	0.0	12.33	12.99	12.00	11.59	11.27	12.50
EOS%	0.27	0.30	0.31	0.28	0.29	0.24	0.28	0.6	11.59	12.15	13.03	12.12	12.03	11.43
BASO#	0.03	0.02	0.03	0.02	0.02	0.03	0.02	0.0	21.55	19.13	21.49	17.27	15.24	21.55
BASO%	0.72	0.62	0.59	0.63	0.55	0.77	0.65	1.3	19.30	16.85	14.94	17.12	15.36	20.05
RBC	0.04	0.04	0.04	0.03	0.03	0.03	0.04	0.1	1.30	1.20	1.51	0.96	0.97	1.03
HGB	0.12	0.14	0.13	0.18	0.16	0.19	0.15	0.3	1.58	1.87	1.88	2.38	2.10	2.73
HCT	0.24	0.26	0.31	0.22	0.22	0.23	0.25	0.5	1.07	1.15	1.45	0.96	0.95	1.04
MCV	0.48	0.49	0.47	0.47	0.48	0.59	0.50	1.0	0.66	0.67	0.64	0.64	0.65	0.79
MCH	0.46	0.55	0.62	0.68	0.58	0.72	0.60	1.2	1.86	2.26	2.53	2.80	2.36	3.02
MCHC	0.62	0.73	0.79	0.93	0.74	0.98	0.80	1.6	1.83	2.20	2.37	2.82	2.24	3.06
RDW%	0.14	0.21	0.17	0.16	0.18	0.20	0.18	0.4	1.12	1.66	1.42	1.24	1.38	1.51
PLT	6.00	6.40	4.20	4.40	3.70	5.20	4.98	10.0	6.40	6.69	5.17	5.12	4.49	6.24

Normal

Lot #s	SD						Historical		CV					
	8273	8273	8329	9019	9019	9075	SD	2 SD	8273	8273	8329	9019	9019	9075
WOC	0.11	0.10	0.11	0.09	0.10	0.10	0.10	0.2	1.54	1.40	1.58	1.26	1.41	1.42
NEUT#	0.08	0.08	0.09	0.07	0.08	0.08	0.08	0.2	1.88	1.99	2.09	1.68	2.02	1.80
NEUT%	0.59	0.89	0.80	0.78	0.76	0.67	0.75	1.5	1.04	1.57	1.37	1.34	1.31	1.14
LYM#	0.06	0.06	0.06	0.07	0.08	0.06	0.07	0.1	3.17	3.17	3.14	3.74	4.30	3.43
LYM%	0.63	0.80	0.68	0.91	1.02	0.77	0.80	1.6	2.38	3.01	2.47	3.49	3.89	2.96
MONO#	0.04	0.04	0.04	0.04	0.05	0.03	0.04	0.1	5.26	5.19	6.78	5.97	7.58	5.31
MONO%	0.52	0.58	0.50	0.60	0.68	0.47	0.56	1.1	4.87	5.39	5.92	6.46	7.33	5.19
EOS#	0.01	0.02	0.01	0.02	0.01	0.01	0.01	0.0	5.26	8.47	7.78	7.21	6.76	7.41
EOS%	0.19	0.22	0.22	0.21	0.20	0.20	0.21	0.4	7.20	8.30	9.13	7.24	6.85	7.46
BASO#	0.02	0.02	0.03	0.03	0.03	0.02	0.02	0.0	8.00	9.88	13.40	10.76	10.44	9.75
BASO%	0.30	0.35	0.41	0.38	0.33	0.32	0.35	0.7	8.40	10.23	13.62	10.95	9.46	9.61
RBC	0.04	0.05	0.05	0.05	0.05	0.04	0.05	0.1	0.96	1.20	1.26	1.17	1.17	0.94
HGB	0.13	0.16	0.16	0.21	0.18	0.23	0.18	0.4	1.11	1.37	1.33	1.76	1.50	1.88
HCT	0.31	0.36	0.36	0.34	0.38	0.39	0.36	0.7	1.01	1.16	1.15	1.05	1.16	1.19
MCV	0.58	0.60	0.51	0.43	0.46	0.63	0.54	1.1	0.78	0.80	0.67	0.57	0.60	0.82
MCH	0.46	0.58	0.57	0.59	0.50	0.59	0.55	1.1	1.63	2.07	2.00	2.12	1.78	2.06
MCHC	0.56	0.69	0.66	0.73	0.64	0.87	0.69	1.4	1.47	1.84	1.76	1.99	1.74	2.33

Para 12[®] Plus Retics

Instrument/Serial Number - Abbott CELL-DYN[®] 3200

Lab Acct Number: 00100
 SAMPLE LAB REPORT
 1234 MAIN STREET
 ANYTOWN, NE USA 68130

Lot Number 9075
 Instrument Number 339
 Shift 1

Report Date 06/15/2009
 Date Received 06/03/2009
 Date From 04/01/2009
 Date To 05/29/2009

	8273	8273	8329	9019	9019	9075	SD	2 SD	8273	8273	8329	9019	9019	9075
RDW%	0.16	0.16	0.17	0.14	0.15	0.20	0.16	0.3	1.44	1.43	1.47	1.18	1.26	1.75
PLT	10.20	11.60	7.90	9.90	7.80	9.10	9.42	18.8	4.21	4.70	3.34	4.19	3.38	3.81

High

Lot #'s	SD						Historical		CV					
	8273	8273	8329	9019	9019	9075	SD	2 SD	8273	8273	8329	9019	9019	9075
WOC	0.27	0.24	0.24	0.28	0.29	0.25	0.26	0.5	1.69	1.51	1.55	1.73	1.80	1.60
NEUT#	0.22	0.19	0.18	0.19	0.20	0.22	0.20	0.4	2.16	1.87	1.86	1.85	1.96	2.18
NEUT%	0.75	0.71	0.67	0.57	0.60	0.74	0.67	1.3	1.18	1.11	1.07	0.90	0.94	1.14
LYM#	0.18	0.11	0.10	0.13	0.11	0.10	0.12	0.2	6.45	4.00	3.27	4.19	3.58	3.36
LYM%	1.01	0.64	0.56	0.63	0.58	0.60	0.67	1.3	5.78	3.70	2.84	3.29	3.04	3.14
MONO#	0.11	0.10	0.07	0.10	0.08	0.10	0.09	0.2	5.64	5.13	3.91	5.71	4.73	6.54
MONO%	0.76	0.57	0.43	0.56	0.48	0.66	0.58	1.2	6.21	4.65	3.72	5.34	4.56	6.71
EOS#	0.03	0.03	0.03	0.03	0.03	0.03	0.03	0.1	5.88	5.31	6.38	5.30	5.88	6.38
EOS%	0.18	0.17	0.20	0.17	0.20	0.17	0.18	0.4	5.66	5.31	6.62	4.86	5.73	5.61
BASO#	0.08	0.05	0.05	0.05	0.05	0.04	0.05	0.1	14.55	8.85	9.80	9.09	9.26	7.55
BASO%	0.48	0.30	0.31	0.29	0.32	0.29	0.33	0.7	13.95	8.98	9.48	8.45	9.50	8.55
RBC	0.07	0.06	0.06	0.06	0.07	0.06	0.06	0.1	1.39	1.20	1.26	1.17	1.37	1.18
HGB	0.23	0.21	0.20	0.33	0.28	0.28	0.26	0.5	1.47	1.35	1.31	1.97	1.65	1.70
HCT	0.54	0.48	0.52	0.49	0.57	0.66	0.54	1.1	1.38	1.22	1.35	1.17	1.35	1.60
MCV	0.61	0.51	0.58	0.45	0.55	0.70	0.57	1.1	0.78	0.65	0.73	0.55	0.66	0.86
MCH	0.44	0.54	0.56	0.74	0.49	0.50	0.55	1.1	1.41	1.74	1.76	2.25	1.47	1.54
MCHC	0.51	0.65	0.66	0.81	0.62	0.72	0.66	1.3	1.28	1.64	1.65	2.02	1.54	1.80
RDW%	0.17	0.17	0.18	0.18	0.15	0.19	0.17	0.3	1.57	1.56	1.66	1.60	1.33	1.75
PLT	15.70	24.90	13.00	20.30	20.70	19.50	19.02	38.0	2.71	4.26	2.16	3.43	3.58	3.39